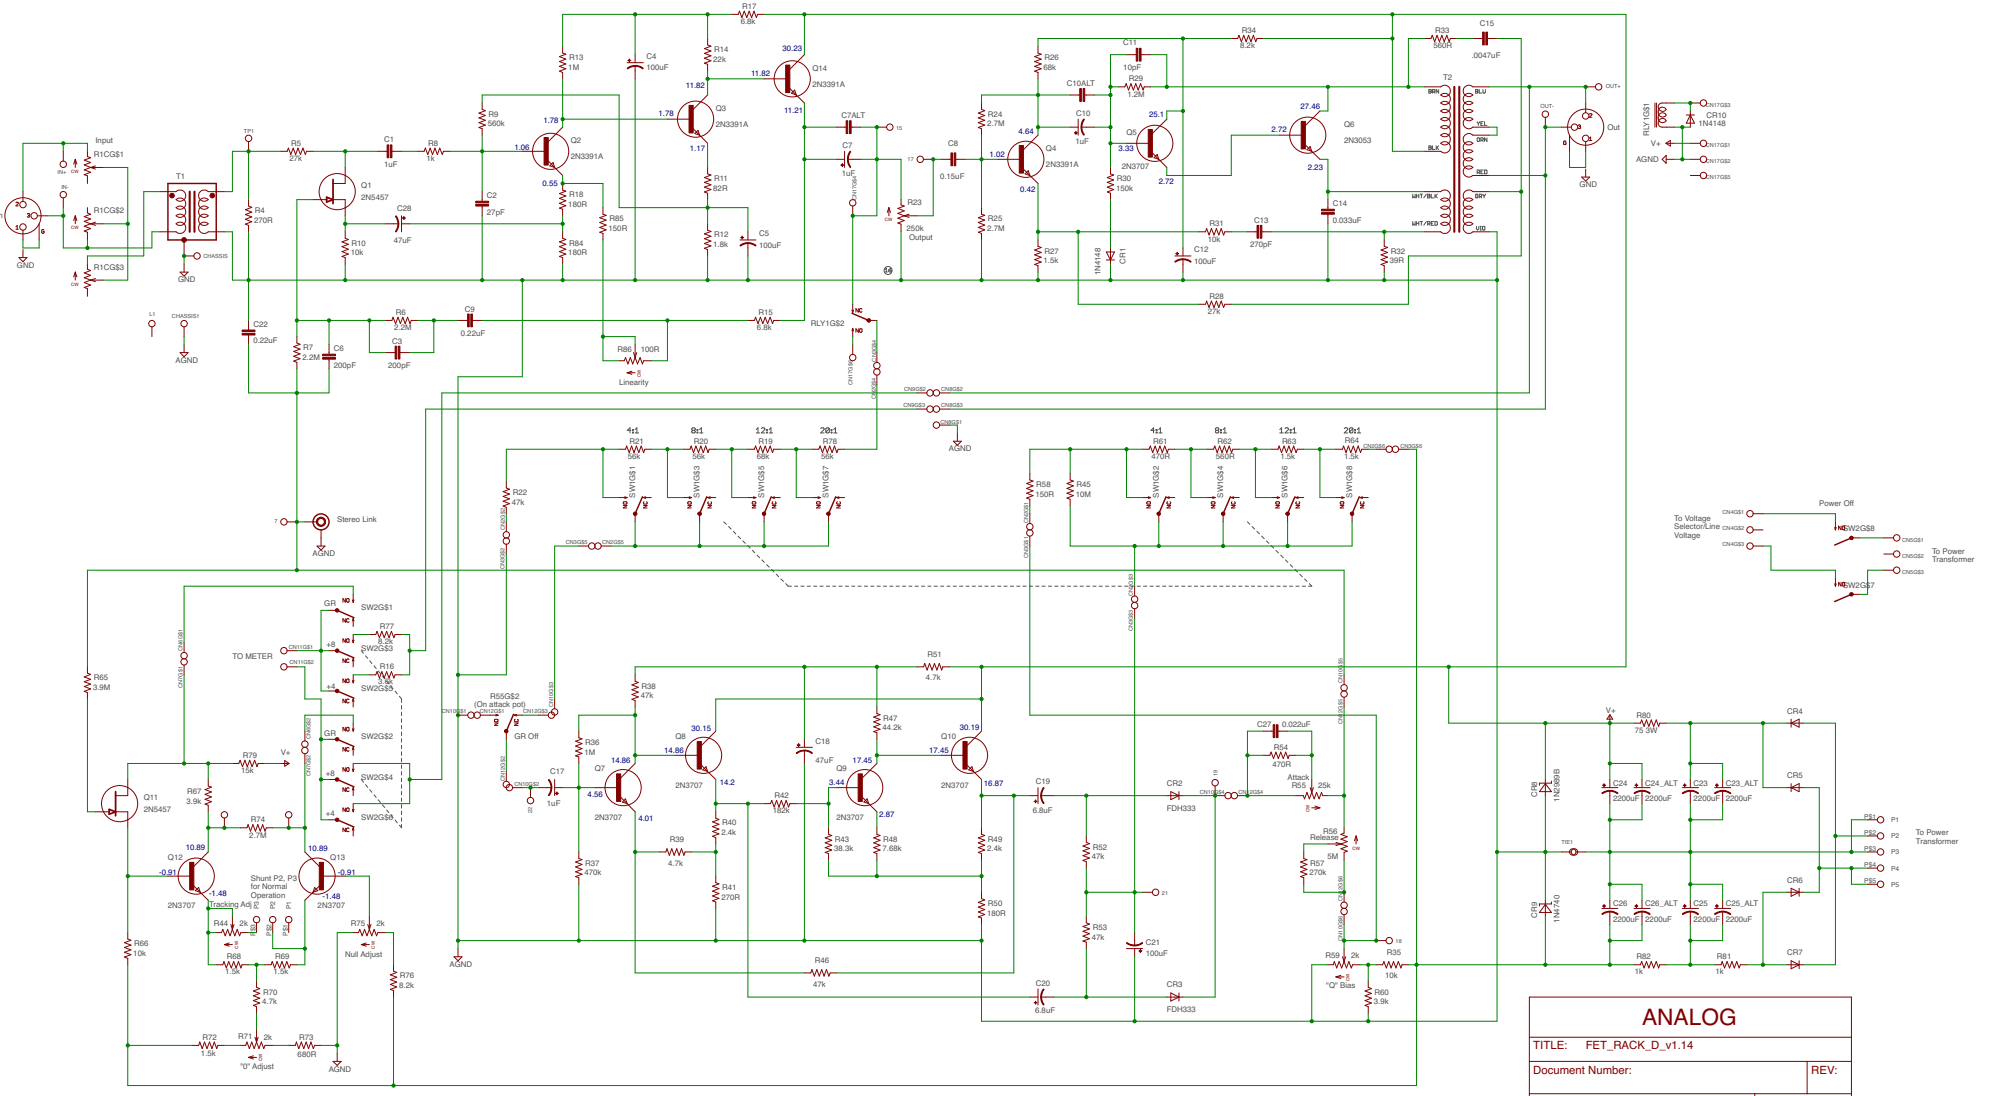

Typical DC Voltages for a calibrated unit warmed for 10 min.